

Impacts of Ignition Furnace Correction Factors Errors to Quality Assurance of Asphalt Mixtures

**PAPA Regional Technical Meetings
March, 2024**

**Derek Nener-Plante, M.S., P.E.
Pavement & Materials Engineer
Resource Center
Office of Innovation Implementation**



U.S. Department of Transportation
Federal Highway Administration



Disclaimers

- The contents of this presentation do not have the force and effect of law and are not meant to bind the public in any way. This presentation is intended only to provide information to the public regarding existing requirements under the law or agency policies.
- The U.S. Government does not endorse products or manufacturers. Trademarks or manufacturers' names appear in this presentation only because they are considered essential to the objective of the presentation. They are included for informational purposes only and are not intended to reflect a preference, approval, or endorsement of any one product or entity.
- All AASHTO & ASTM standards mentioned in this presentation content are private, voluntary standards and compliance with them are not required under Federal law.
- Unless noted otherwise, FHWA is the source for all images in this presentation.



Acknowledgements

- Casey Nash and Ryan Robinson from MaineDOT
- Dennis Dvorak from FHWA-Resource Center



Abbreviations and Acronyms

- AASHTO – American Association of State Highway and Transportation Officials
- CF – Correction factor
- JMF – Job mix formula
- LCP – Light capital pavement
- NMAS – Nominal maximum aggregate size
- PWL – percent within limits
- UTB – Ultra-thin bonded



Why do you care?

What are you going to get out of this?

Give context for the **significant impact of errors** in correction factors for ignition furnaces

- Impacts accurate and fair **acceptance** by agencies
- Impacts **quality control** assessments by contractors
- Impacts proper and fair payment for asphalt mixtures



Why do you care?

What are you going to get out of this?

Topics for discussion:

- Background
 - AASHTO T 308
 - MaineDOT practice
- Results
 - All CF
 - CF comparisons
 - Impact on QA
 - Simulations
 - Real Lot data





U.S. Department of Transportation
Federal Highway Administration




Background

AASHTO T 308 – Ignition Furnace

- Used by most agencies and contractors to determine asphalt content
- Correction factor key to adjust for aggregate burn off and breakdown at high temperatures

Entity preparing ignition furnace correction factors
(Source: NCHRP 09-56)

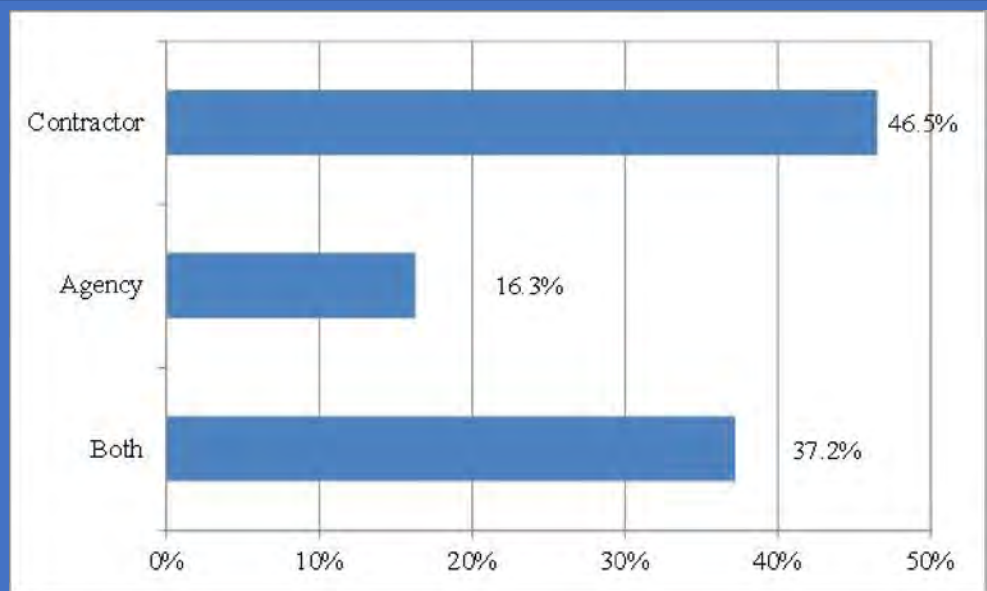

AASHTO T 308 – Correction Factors


- “A1.1. Asphalt binder content results may be affected by the type of aggregate in the mixture and the ignition furnace. **Therefore, asphalt binder and aggregate correction factors must be established by testing a set of correction specimens for each job mix formula (JMF) mix design.** Correction factor(s) must be determined before any acceptance testing is completed and repeated each time a change in the mix ingredients or design occurs. **Any changes greater than 5 percent in stockpiled aggregate proportions should require a new correction factor.”**
- NCHRP 09-56 Variability of Ignition Furnace Correction Factors
 - “Although not recommended in the AASHTO T 308 standard, sharing correction factors between different furnaces should not be a significant problem when low correction factor aggregates (of 0.1% or less) are used. For higher mass loss aggregates (1.0% and larger), **sharing correction factors should not be allowed.** As the CF increases from 0.1% to 1.0%, the errors caused by sharing CFs will certainly increase.”




Background: Acceptance Sampling Practice



Sampling from the paver hopper onsite



Secured by agency personnel.

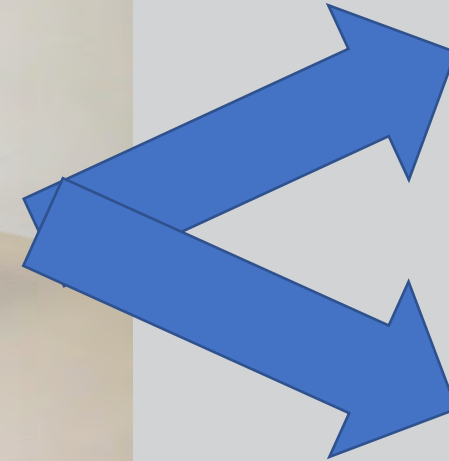

Lab #1
(Central Lab)

Lab #2
(Regional Lab)

Transported by contractor to one of two MaineDOT labs

Background: Correction Factor Practice

- Correction factor generated by MaineDOT for each 'base' JMF for each furnace per AASHTO T 308
 - 'Base' considered to be aggregate and RAP skeleton and binder aim – can vary binder grade, additives, etc.
- Lab batches two samples for design using component aggregate, virgin binder content, and RAP
 - Actual binder mass added is recorded and used.
- One sample is split into four AASHTO T308 tests and correction factor generated from average of four samples
- Second sample is shipped to second lab for their potential use in dispute process – split and tested a similar way in another furnace.



Unique Data Analysis Opportunity

- Database containing the following:
 - Mix design
 - Date correction factor performed
 - Laboratory
 - Furnace ID
 - Correction factor
- Opportunity to:
 - Analyze distribution of correction factors
 - Compare CF between labs and furnace generated using same process

Comparison ID	REF ID	Furnace 1	Furnace 1 Date	Furnace Loss 1	Furnace 2	Furnace 2 Date	Furnace Loss 2
001	16018	FRPT-NCAT1.1	31-Aug-18	0.80	BGR-NCAT3.1	17-Jun-19	0.70
002	17079	BGR-NCAT2	12-Sep-19	0.35	FRPT-NCAT1.1	09-Oct-19	0.53
003	17085	BGR-NCAT1	18-Sep-19	0.52	FRPT-NCAT2	03-Sep-19	0.68
004	17105	FRPT-NCAT2	04-Sep-19	0.35	BGR-NCAT1	22-Jun-19	0.31
005	17907	BGR-NCAT2	03-Sep-19	0.4	FRPT-NCAT1.1	18-Jun-19	0.44
006	18007	BGR-NCAT3.1	15-Jun-19	1.13	FRPT-NCAT2	18-Jun-19	1.12
007	18060	FRPT-NCAT2	31-Aug-18	0.43	BGR-NCAT3.1	17-Jun-19	0.5
008	18066	BGR-NCAT4	16-Aug-18	0.47	FRPT-NCAT3	10-Oct-18	0.37
009	19001	BGR-NCAT4	17-Jun-19	0.32	FRPT-NCAT3	03-May-19	0.29
010	19001	FRPT-NCAT3	03-May-19	0.29	FRPT-NCAT2	07-Aug-20	0.27
011	19001	BGR-NCAT4	17-Jun-19	0.32	FRPT-NCAT2	07-Aug-20	0.27
012	19003	BGR-NCAT2	17-Sep-20	0.44	FRPT-NCAT3	02-Jul-19	0.42
013	19003	FRPT-NCAT3	02-Jul-19	0.42	FRPT-NCAT1.1	13-May-19	0.38
014	19003	BGR-NCAT2	17-Sep-20	0.44	FRPT-NCAT1.1	13-May-19	0.38
015	19019	BGR-NCAT3.1	19-Jun-19	0.24	FRPT-NCAT2	22-Oct-20	0.14
016	19020	FRPT-NCAT3	12-Jul-19	0.34	BGR-NCAT1	28-Jun-19	0.3
017	19024	BGR-NCAT3.1	01-Aug-19	0.3	FRPT-NCAT2	30-Apr-19	0.27
018	19025	FRPT-NCAT2	27-Apr-19	0.33	BGR-NCAT1	22-Oct-19	0.29
019	19029	BGR-NCAT3.1	23-Nov-20	0.33	FRPT-NCAT1.1	12-Jul-19	0.33
020	19034	FRPT-NCAT3	14-Jun-19	0.33	BGR-NCAT1	03-May-20	0.40



Unique Data Analysis Opportunity

This study:

Mix Design	<i>Same</i>	
Correction Factor Procedure	<i>Same</i>	
Furnace Manufacturer	<i>Same</i>	
Staff training	<i>Same</i>	
Ignition Furnace		<u>Different</u>
Laboratory		<u>Different</u>

Real life:

Mix Design	<i>Same</i>	
Correction Factor Procedure		<u>Different</u>
Furnace Manufacturer		<u>Different</u>
Staff training		<u>Different</u>
Ignition Furnace		<u>Different</u>
Laboratory		<u>Different</u>

This is a best-case scenario for AASHTO T308 correction factor differences.






U.S. Department of Transportation
Federal Highway Administration



Results


Correction Factor Distribution

- 2018-2022
- Typical factors between 0.3% – 0.5%
- Clear difference between LCP and UTB
 - Impact of recycled materials, aggregate types, and fines

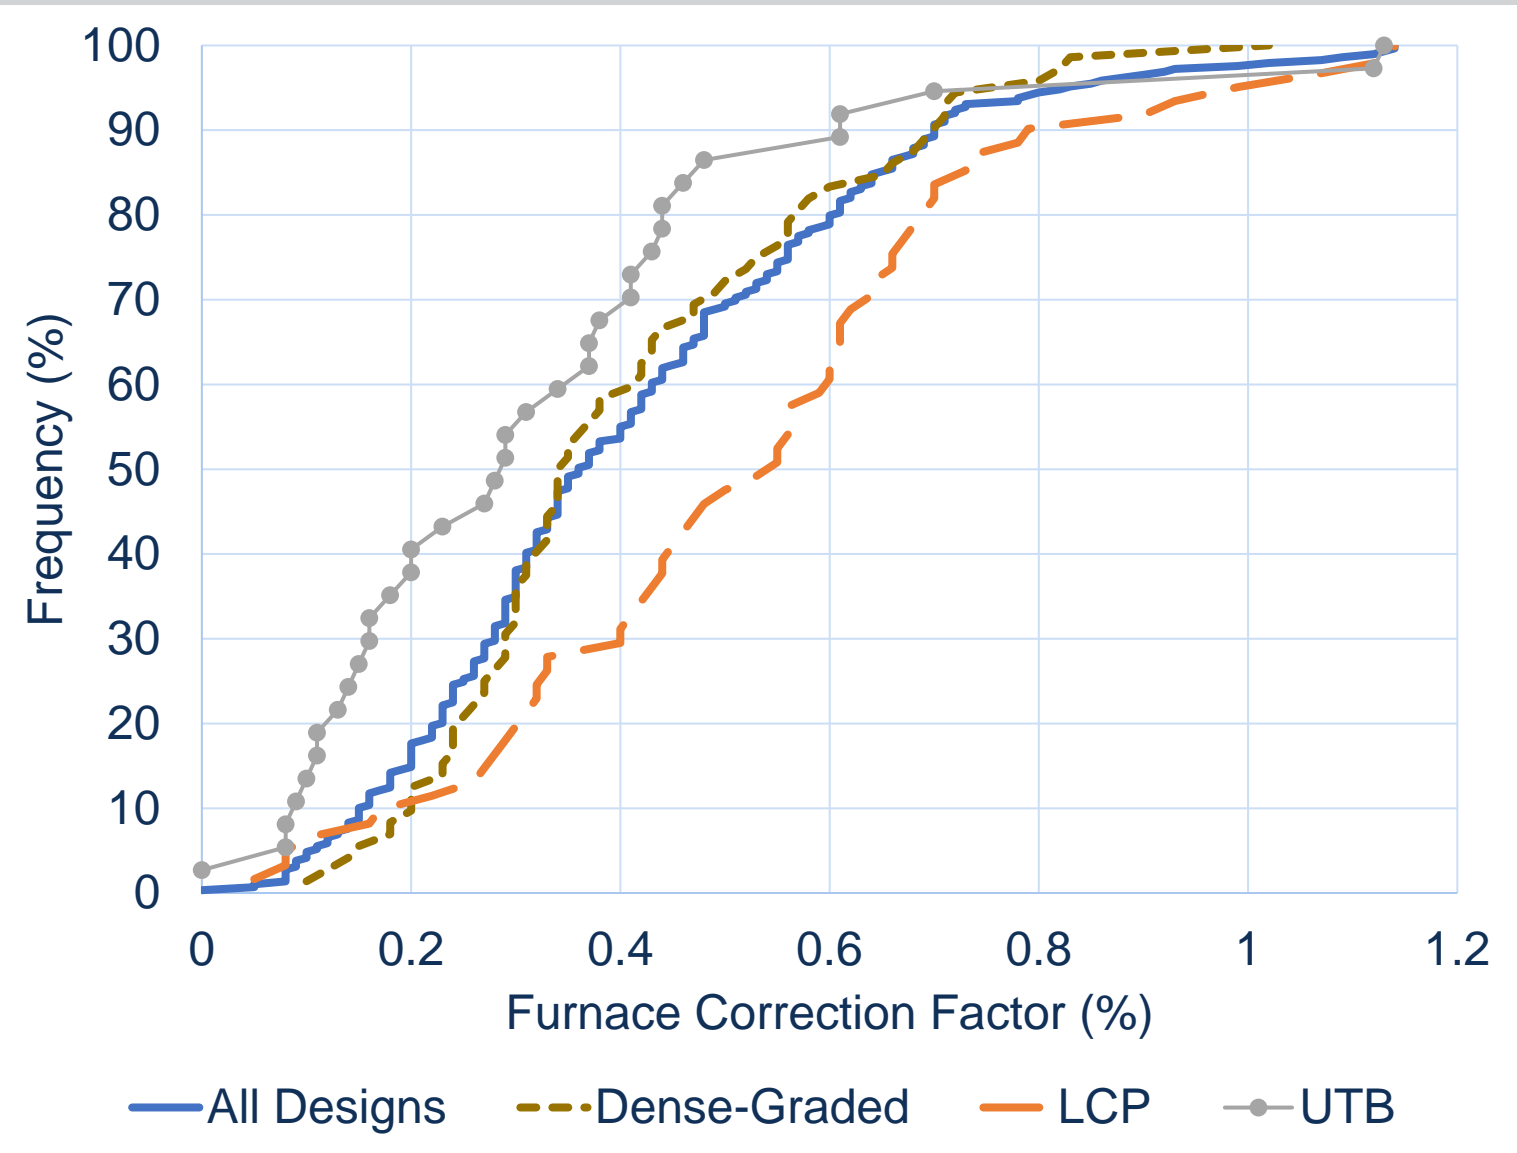

Correction Factor Distribution

- 2018-2022
- No clear impact of NMAS

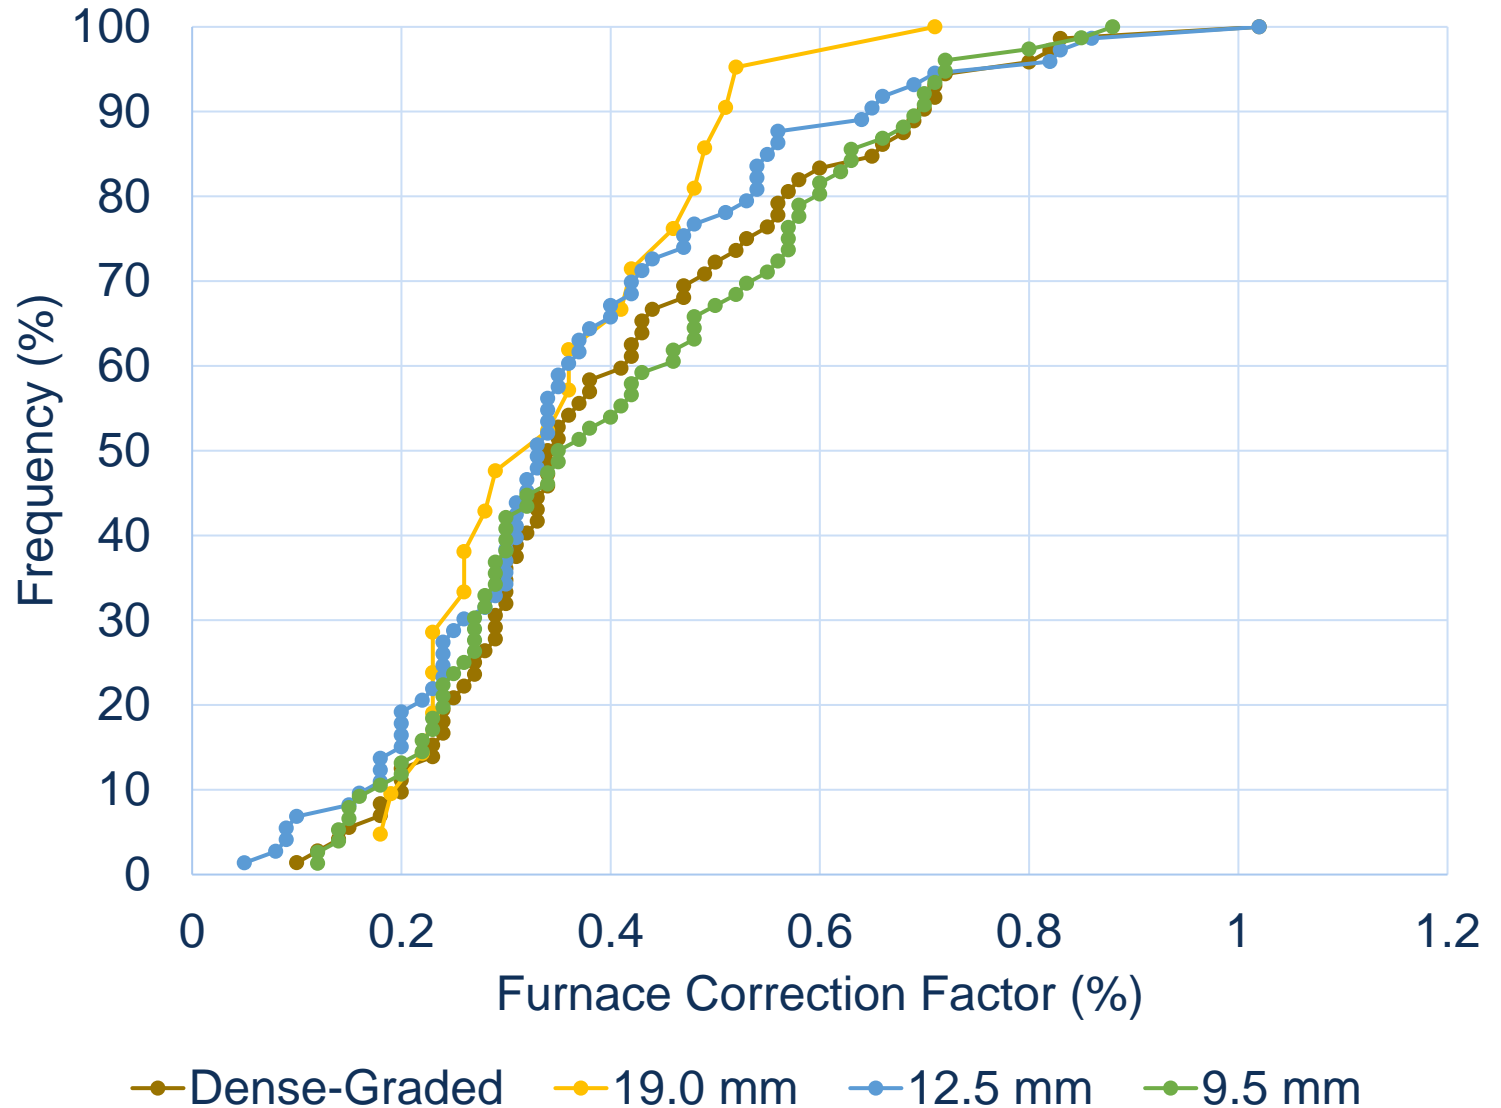

Correction Factor Comparisons


- 75 comparisons between different furnaces for the same mixture design.
 - 13 from the same lab / 62 from different labs
- Absolute differences

Comparison ID	REF ID	Furnace 1	Furnace 1 Date	Furnace Loss 1	Furnace 2	Furnace 2 Date	Furnace Loss 2
001	16018	FRPT-NCAT1.1	31-Aug-18	0.80	BGR-NCAT3.1	17-Jun-19	0.70
002	17079	BGR-NCAT2	12-Sep-19	0.35	FRPT-NCAT1.1	09-Oct-19	0.53
003	17085	BGR-NCAT1	18-Sep-19	0.52	FRPT-NCAT2	03-Sep-19	0.68
004	17105	FRPT-NCAT2	04-Sep-19	0.35	BGR-NCAT1	22-Jun-19	0.31
005	17907	BGR-NCAT2	03-Sep-19	0.4	FRPT-NCAT1.1	18-Jun-19	0.44
006	18007	BGR-NCAT3.1	15-Jun-19	1.13	FRPT-NCAT2	18-Jun-19	1.12
007	18060	FRPT-NCAT2	31-Aug-18	0.43	BGR-NCAT3.1	17-Jun-19	0.5
008	18066	BGR-NCAT4	16-Aug-18	0.47	FRPT-NCAT3	10-Oct-18	0.37
009	19001	BGR-NCAT4	17-Jun-19	0.32	FRPT-NCAT3	03-May-19	0.29
010	19001	FRPT-NCAT3	03-May-19	0.29	FRPT-NCAT2	07-Aug-20	0.27
011	19001	BGR-NCAT4	17-Jun-19	0.32	FRPT-NCAT2	07-Aug-20	0.27
012	19003	BGR-NCAT2	17-Sep-20	0.44	FRPT-NCAT3	02-Jul-19	0.42
013	19003	FRPT-NCAT3	02-Jul-19	0.42	FRPT-NCAT1.1	13-May-19	0.38
014	19003	BGR-NCAT2	17-Sep-20	0.44	FRPT-NCAT1.1	13-May-19	0.38
015	19019	BGR-NCAT3.1	19-Jun-19	0.24	FRPT-NCAT2	22-Oct-20	0.14
016	19020	FRPT-NCAT3	12-Jul-19	0.34	BGR-NCAT1	28-Jun-19	0.3
017	19024	BGR-NCAT3.1	01-Aug-19	0.3	FRPT-NCAT2	30-Apr-19	0.27
018	19025	FRPT-NCAT2	27-Apr-19	0.33	BGR-NCAT1	22-Oct-19	0.29
019	19029	BGR-NCAT3.1	23-Nov-20	0.33	FRPT-NCAT1.1	12-Jul-19	0.33



Difference in CF – Cumulative Distribution

- Avg. Difference = 0.10
- Median Difference = 0.07
- 75th percentile = 0.14
- Different labs saw the highest differences

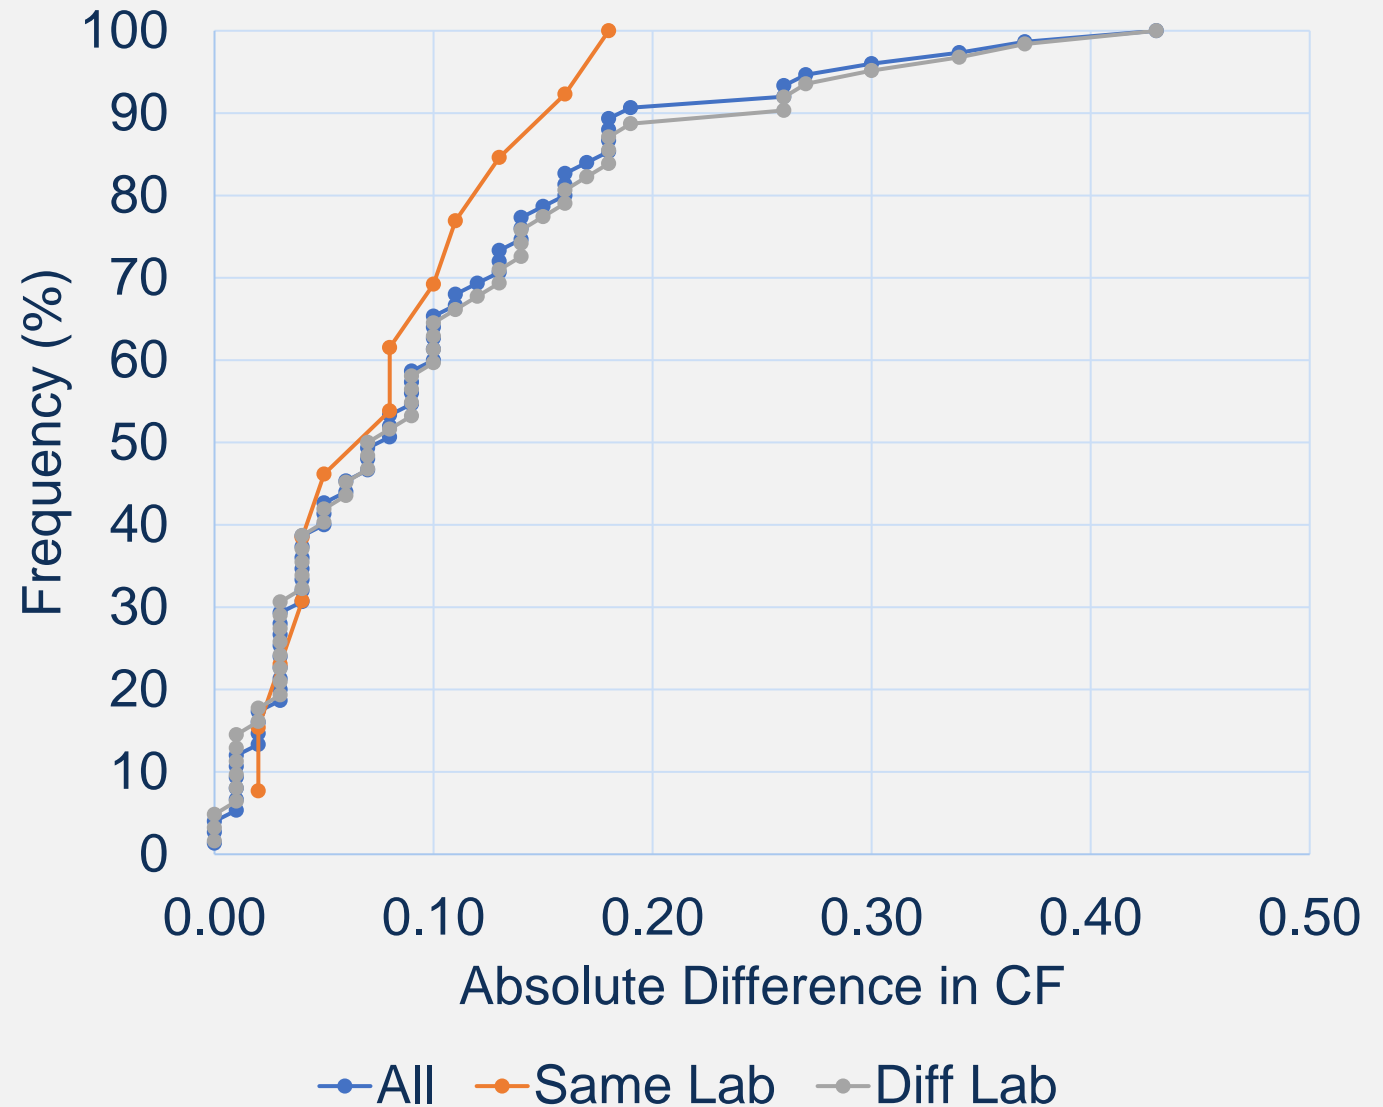

Background: MaineDOT PWL Acceptance

- MaineDOT uses PWL and AASHTO pay equation (90 PWL = 1.0 pay)
- Agency-only results
- Asphalt content equals 25% of composite payfactor
- Typical lot (6 sublots) of 4500 tons at \$100/ton used for cost analysis
- Asphalt content tolerance of 0.4% from mix design aim as LSL and USL

QA Impacts based upon three CF error values:


- 0.07 (Median)
- 0.10 (Average)
- 0.14 (75th percentile)




Scenarios to Simulate CF Impact

Run for positive bias and negative bias, positive shown only as example


Scenario 1:
Lot on aim with typical standard deviation (90 PWL).

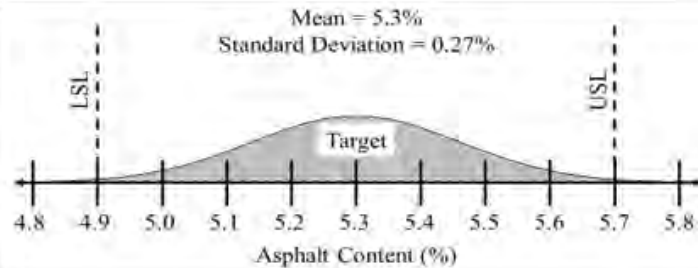


Scenario 2:
Lot average 0.1% higher than target with tighter standard deviation to achieve 90 PWL.

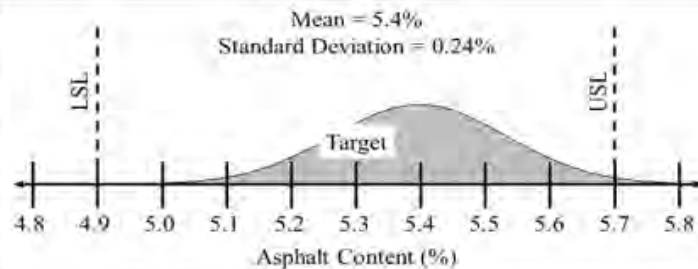


Scenario 3:
Lot average 0.2% higher than target with tighter standard deviation to achieve 90 PWL.

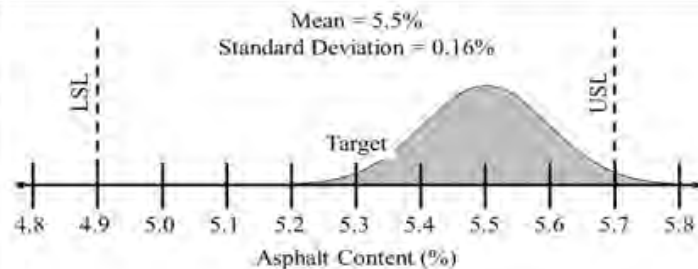


Scenario 4:
Lot average 0.3% higher than target with tighter standard deviation to achieve 90 PWL.

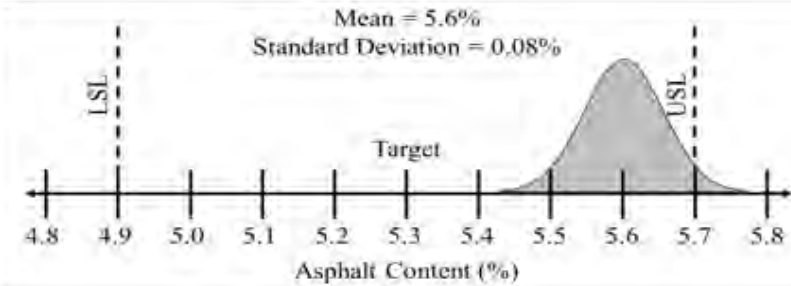


Scenario 5:
Lot average 0.1% high with typical standard deviation.

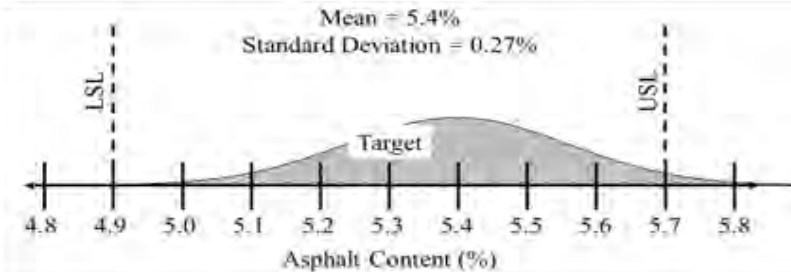

Scenario 6:
Lot average 0.2% high with typical standard deviation.

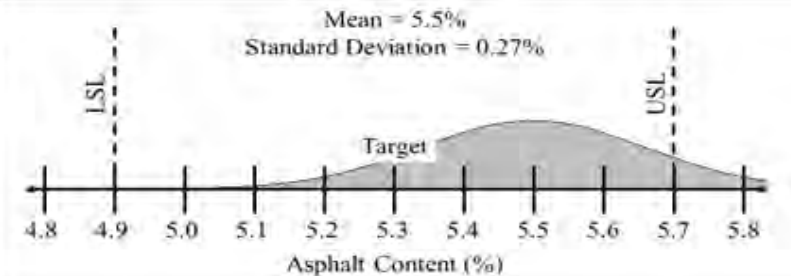


Scenario 7:
Lot average 0.3% high with typical standard deviation.

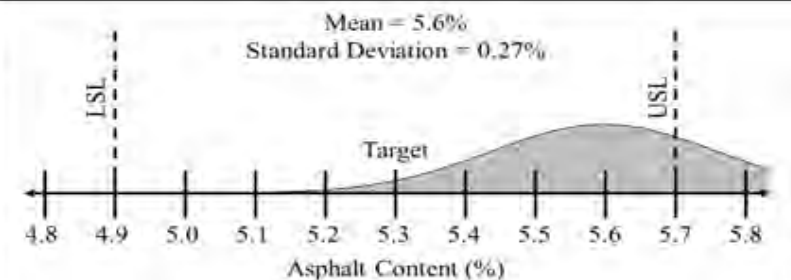


Scenarios to Simulate CF Impact

Run for positive bias and negative bias, positive shown only as example

Scenario 4:
Lot average 0.3% higher than target with tighter standard deviation to achieve 90 PWL.

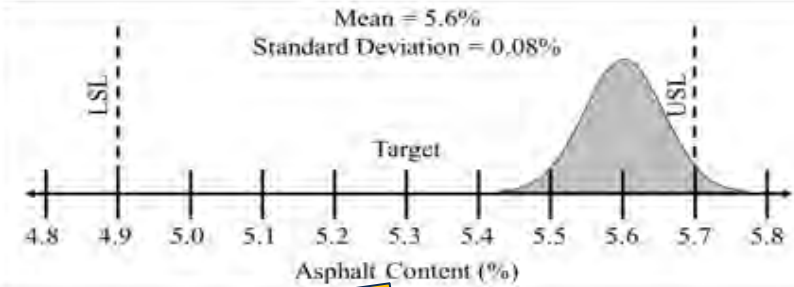


Scenario 5:
Lot average 0.1% higher than target with typical standard deviation to achieve 90 PWL.

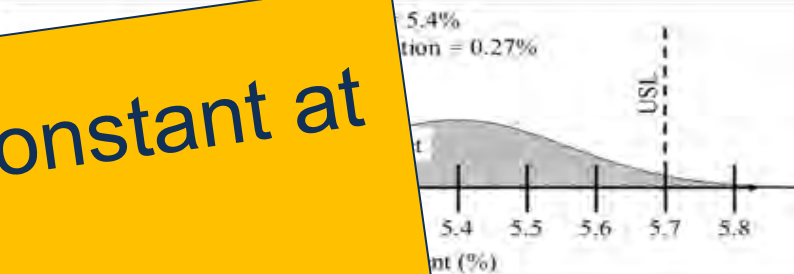


Scenarios 1-4 = Starting PWL held constant at 90 with different averages

Scenarios 5-7 = Lot standard deviation held constant with different averages

Scenario 6:
Lot average 0.2% higher than target with typical standard deviation to achieve 90 PWL.

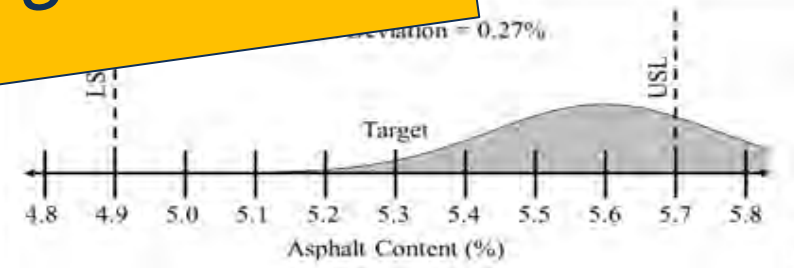

Scenario 1:
Lot on aim with typical standard deviation (90 PWL).

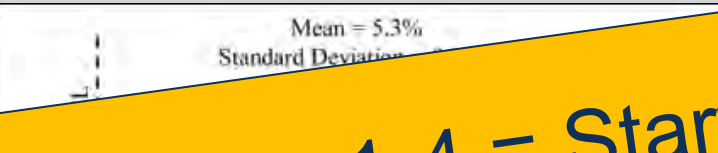

Scenario 2:
Lot average 0.1% higher than target with tighter standard deviation to achieve 90 PWL.



Scenario 3:
Lot average 0.2% higher than target with tighter standard deviation to achieve 90 PWL.



PWL Error

(Positive Bias)

- Assumes no adjustment by the contractor to Acceptance results as that cannot be simulated
- Significant effects, especially when the original average value is off the stated aim

ΔPWL Based Per Condition		Scenarios 1-4				Scenarios 5-7		
		Average Lot Asphalt Content				Average Lot Asphalt Content		
		On Aim	Aim + 0.1%	Aim + 0.2%	Aim + 0.3%	Aim + 0.1%	Aim + 0.2%	Aim + 0.3%
Change in CF	-0.07	-1.8	-7.5	-11.8	-26.4	-6.7	-8.7	-12.6
	+0.07	-1.8	4.5	7.8	10.1	3.3	7.7	-31.6
	-0.10	-3.6	-12.5	-19.9	-44.5	-11.4	-13.9	-22.0
	+0.10	-3.6	4.9	9.8	10.1	3.6	10.9	-3.6
	-0.14	-7.1	-16.5	-26.4	-57.8	-15.1	-17.9	-27.5
	+0.14	-7.1	4.2	10.1	10.1	3.0	12.5	1.2



ΔPayment (Positive Bias)

- Assumes no adjustment by the contractor to Acceptance results as that cannot be simulated
- 1% = \$4500 in scenario

Change in Overall Lot Payment Per Condition		Scenarios 1-4				Scenarios 5-7		
		Average Lot Asphalt Content				Average Lot Asphalt Content		
		On Aim	Aim + 0.1%	Aim + 0.2%	Aim + 0.3%	Aim + 0.1%	Aim + 0.2%	Aim + 0.3%
Change in CF	+0.07	-0.2%	-1.0%	-1.5%	-3.3%	-0.8%	-1.1%	-1.2%
	-0.07	-0.2%	0.6%	1.0%	1.3%	0.4%	1.0%	1.1%
	+0.10	-0.5%	-1.6%	-2.5%	-5.6%	-1.4%	-1.7%	-1.9%
	-0.10	-0.5%	0.6%	1.2%	1.3%	0.4%	1.4%	1.7%
	+0.14	-0.9%	-2.1%	-3.3%	-7.2%	-1.9%	-2.2%	-2.4%
	-0.14	-0.9%	0.5%	1.3%	1.3%	0.4%	1.6%	2.1%




Actual Lot Analysis

- Three major designs evaluated with larger CF differences – 32 total lots
 - Design A (9.5mm Fine-Graded w/ RAP) – CF difference = 0.30
 - Design B (12.5 mm Coarse-Graded w/RAP) – CF difference = 0.37
 - Design C (12.5 mm Coarse-Graded w/RAP) – CF difference = 0.43

Design	Average Original PWL	Average Altered PWL (subtract error)	Average Altered PWL (add error)	Average PWL Error
A	70.6	66.9	43.0	19.4
B	93.1	31.9	77.5	39.7
C	65.8	45.8	48.1	18.9



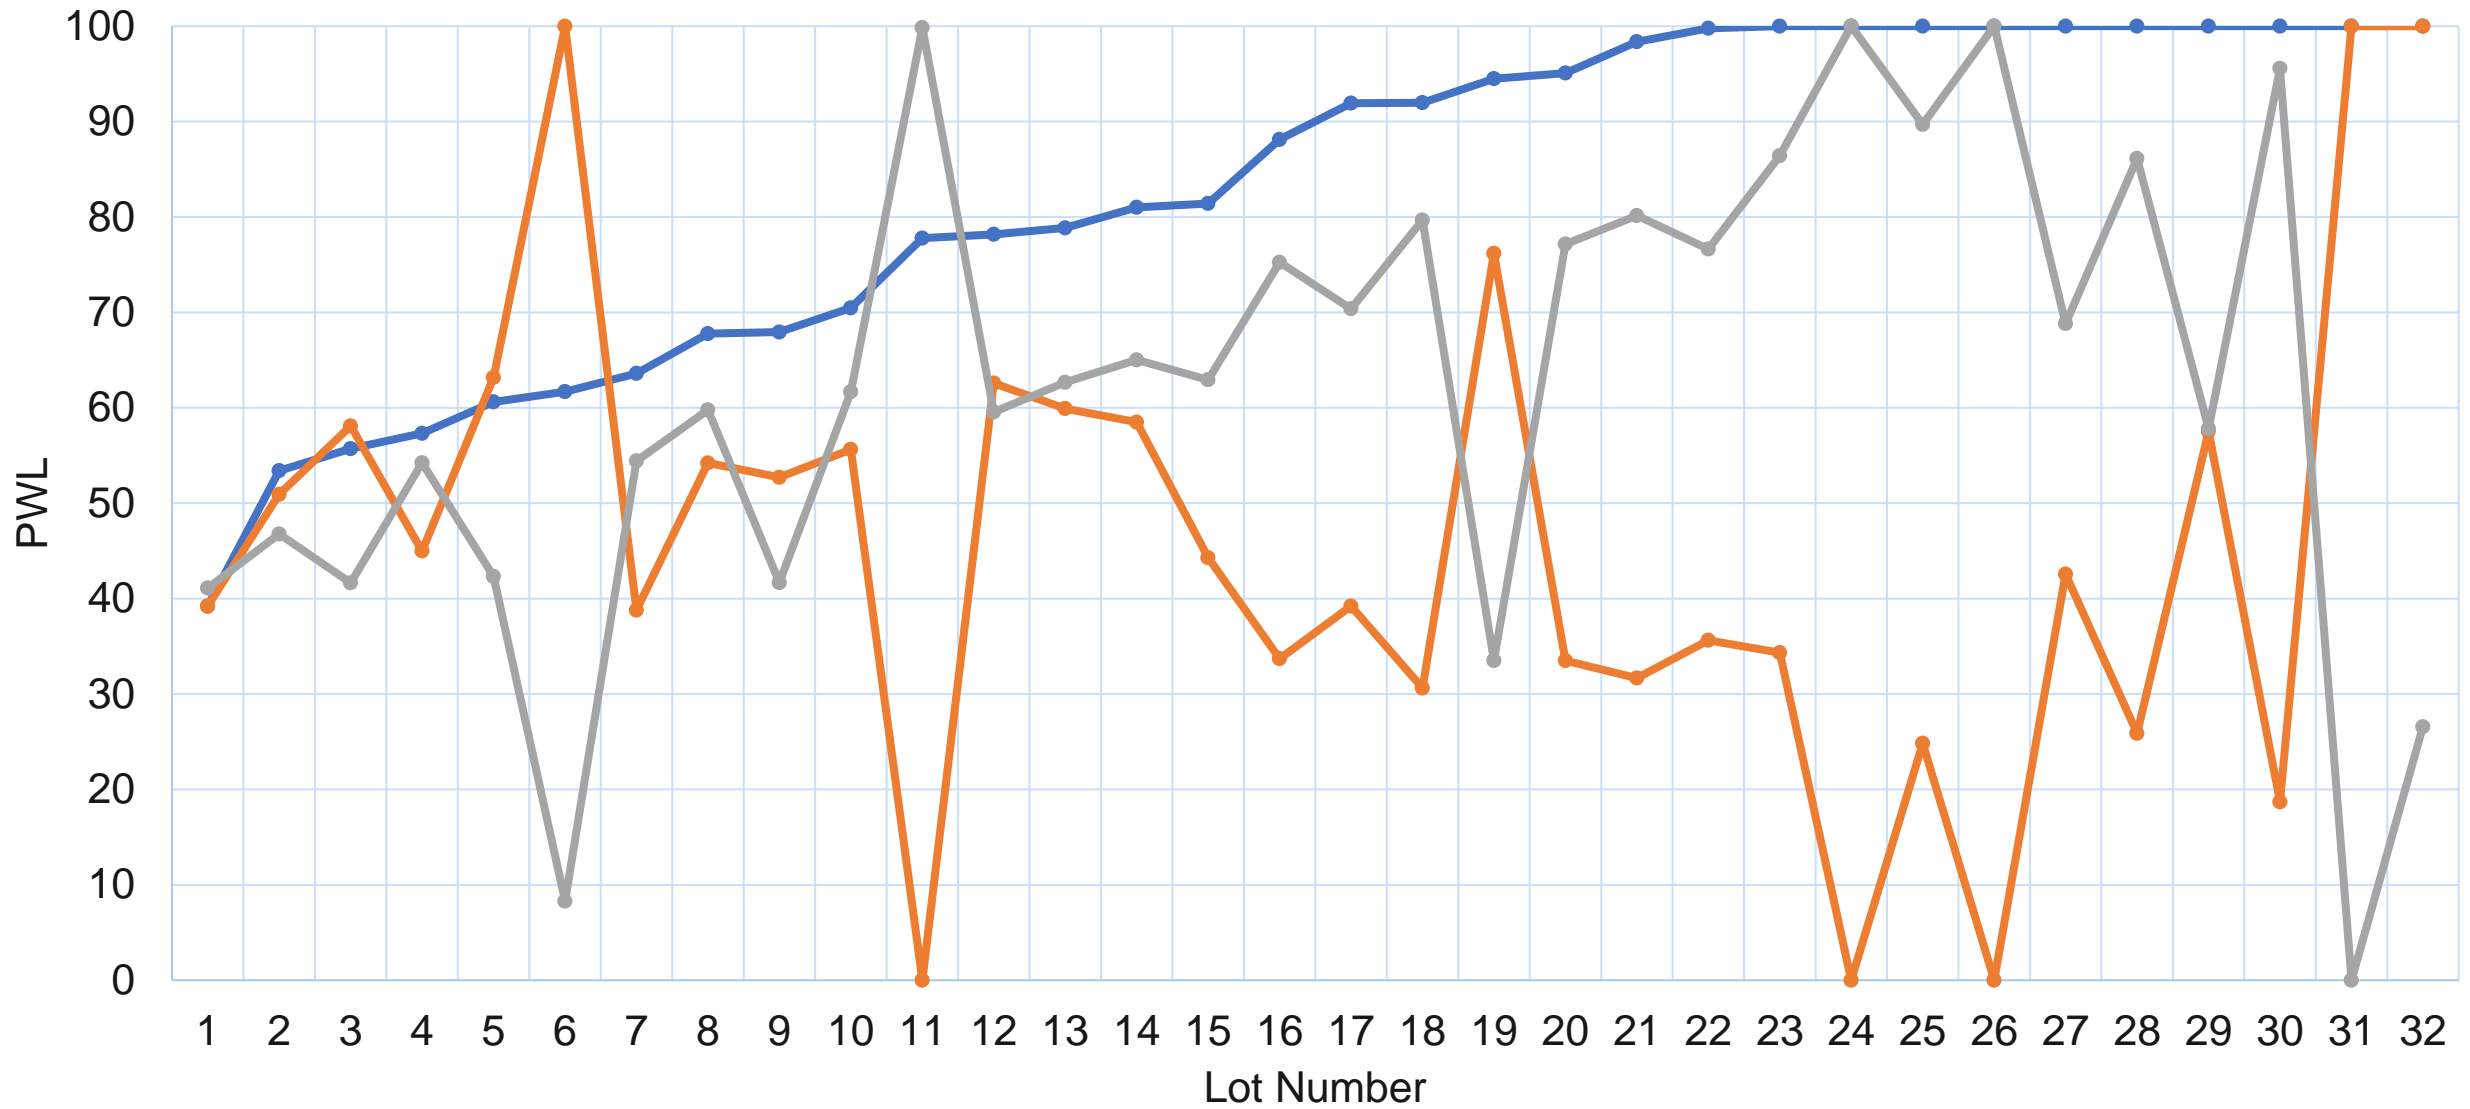

Actual Lot Data

Adjusted PWL (Added Error)

Adjusted PWL (Subtracted Error)



Findings

- Effect of mixture type evident in CF's for MaineDOT mixtures
- Bias observed between CF generated for different furnaces if the same design
 - Range in values for Maine aggregates (0.07 – 0.14 range)
 - Differences smaller than observed than in national studies (typically with higher loss and absorptive aggregates)
- Differences in CF can cause significant impacts to Acceptance and Quality Control functions if accurate CF not generated
 - Observed in statistical acceptance program depending on the conditions
 - Effect can be made worse when production is off the aim





U.S. Department of Transportation
Federal Highway Administration

Questions?

Thank you for your attention!



Derek Nener-Plante
Pavement and Materials Engineer
derek.nenerplante@dot.gov